



INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

<p>(51) International Patent Classification ⁶ : A61G 7/00, 7/057, A47C 19/04</p>	<p>A2</p>	<p>(11) International Publication Number: WO 99/15126 (43) International Publication Date: 1 April 1999 (01.04.99)</p>
<p>(21) International Application Number: PCT/US98/20002 (22) International Filing Date: 23 September 1998 (23.09.98) (30) Priority Data: 60/059,772 23 September 1997 (23.09.97) US 09/120,125 22 July 1998 (22.07.98) US (71) Applicant: HILL-ROM, INC. [US/US]; 1096 State Route 46 East, Batesville, IN 47006-9167 (US). (72) Inventors: ALLEN, E., David; 7513 South Dwyer, Okdana, OH 45053 (US). KRAMER, Kenneth, L.; 6769 West Bloomington Street, St. Paul, IN 47272 (US). WUKU-SICK, Peter, M.; 20157 Five Point Road, Batesville, IN 47006 (US). MEYER, Eric, R.; 4185 County Line Road, Greensburg, IN 47240 (US). BRANSON, Gregory, W.; 323 Woodfield Drive, Batesville, IN 47006 (US). ULRICH, David, J.; 22186 Ester Ridge Road, Sunman, IN 47041 (US). THOMAS, James, M., C.; 1486 Greenshade Way, Mt. Pleasant, SC 29464 (US). DANIEL, Paul, M., III; 2425 Venetian Way, Burlington, KY 41005 (US). ZWINK, Dennis, R.; 27105 Enochsburg Road, Batesville, IN 47006 (US).</p>		<p>(74) Agent: NIEDNAGEL, Timothy, E.; Barnes & Thornburg, 11, South Meridian Street, Indianapolis, IN 46204 (US). (81) Designated States: AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CU, CZ, DE, DK, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, UA, UG, UZ, VN, YU, ZW, ARIPO patent (GH, GM, KE, LS, MW, SD, SZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG).</p> <p>Published <i>Without international search report and to be republished upon receipt of that report.</i></p>
<p>(54) Title: HOSPITAL BED HAVING A RETRACTING FOOT SECTION</p> <p>(57) Abstract</p> <p>A bed having a foot prop (56) on a adjustable length deck foot section (52) and a mattress (20) with a length and thickness adjustable foot section (16) and a thickness adjustable heel section. The adjustability of the deck (10) and the mattress (20) allows sizing of the bed to the occupant as well as heel management. The foot prop (56) is also adjustable.</p>		

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece			TR	Turkey
BG	Bulgaria	HU	Hungary	ML	Mali	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MN	Mongolia	UA	Ukraine
BR	Brazil	IL	Israel	MR	Mauritania	UG	Uganda
BY	Belarus	IS	Iceland	MW	Malawi	US	United States of America
CA	Canada	IT	Italy	MX	Mexico	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NE	Niger	VN	Viet Nam
CG	Congo	KE	Kenya	NL	Netherlands	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NO	Norway	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	NZ	New Zealand		
CM	Cameroon			PL	Poland		
CN	China	KR	Republic of Korea	PT	Portugal		
CU	Cuba	KZ	Kazakhstan	RO	Romania		
CZ	Czech Republic	LC	Saint Lucia	RU	Russian Federation		
DE	Germany	LI	Liechtenstein	SD	Sudan		
DK	Denmark	LK	Sri Lanka	SE	Sweden		
EE	Estonia	LR	Liberia	SG	Singapore		

HOSPITAL BED HAVING A RETRACTING FOOT SECTION

Background and Summary of the Invention

5 The present invention relates generally to adjustable beds and more specifically to a bed having an improved adjustable foot section.

 There are many known bed designs that have adjustable foot sections. On beds that convert from a planar bed configuration to an upright chair configuration, the foot section is generally shortened as the foot section rotates from a horizontal to a
10 vertical position. There are also beds having adjustable lengths wherein an attendant physically repositions the head or foot section of the bed to the desired length. These designs include a sliding telescopic foot section as well as a folding foot section equivalent to a "lazy boy" design. It is also known to deflate the foot section of the mattress when converting from a bed to a chair. For short occupants, there exists a
15 need for adjustment of the foot prop or board in the chair position shorter than that attended by adjusting the length of the foot section.

 The ability to adjust the length of the foot section independent of converting from a bed to a chair is also important. This would assist in maneuvering the bed in a confined locations during patient transport. It also allows the bed length
20 to be customized to a patient's size. If a foot prop is provided at the end of the foot section, the adjustment of the foot section and the prop would prevent patient migration across the support surface of the bed. It would also provide support for the feet to thereby improve the patient's feeling of security. It could also be used in the prevention of peripheral neuropathy ("foot drop"). Positioning the end of the mattress
25 relative to the patient substantially increases the ability to provide heel management. Heel management is wherein the heel is supported by the thigh and the calf and the heel has reduced pressure contact with the mattress.

 Certain individuals who are confined to bed for an extended period of time are vulnerable to skin breakdown on the back of the heel. Protection of the skin
30 in this area is important if initial indications of tissue failure are observed. If the breakdown process has progressed to a point of ulceration, protection of the heel area of the patient is essential to healing.

-2-

Reducing or eliminating the time an individual spends in a supine position will protect the heel area, although it may increase the risk of skin failure on other areas of the foot and body. The current practice for protecting the heel area of a patient while in the supine position utilizes foot support to reduce or eliminate pressure and shear on the back of the heel. Such support is often provided by placing an ordinary pillow or folded towel under a calf area of the patient's legs. Several different foam boot designs are known that strap to the leg or foot to reduce the effects of heel pressure. In addition, a conventional mattress is known in which removable sections are provided in a foot area.

10 All of these conventional support methods require a caretaker to add or remove components from the bed in order to control pressure on the heels of the patient. Components which are removed from the bed have the potential to get lost or mislaid. Components that are added to the bed provide an extra cost associated with the purchasing, cleaning, and disposal of the added components. There is also a cost
15 in time for the caregiver who must go through multiple steps to initiate and maintain the support of the device.

The present invention provides a bed capable of achieving these goals. The bed includes a deck having a foot section of a variable length along the plane of the foot section. A foot prop is mounted to a first end of the foot section and extends
20 transverse to the plane of the foot section. A mattress on the deck has a foot portion of adjustable length along the plane of the foot portion and variable thickness transverse to the plane of the foot portion. A heel portion of the foot portion of the mattress adjacent the foot prop has a thickness variable independent of the thickness of the remainder of the foot portion. The foot portion of the mattress includes a plurality
25 of variable length elements separated by a plurality of variable thickness elements. The variable length elements are connected to operate simultaneously and the variable thickness elements are connected to operate simultaneously and both operate independent of the heel portion. Preferably, the heel portion, the variable length elements and the variable thickness elements each include one or more bladders which
30 are inflatable and deflatable.

To achieve a chair bed, the foot section of the deck is pivotally mounted to the remainder of the deck. A first actuator varies the length of the foot

-3-

section of the deck, a second actuator pivots the foot section of the deck and a third actuator varies the length of the foot portion of the mattress. A fourth actuator varies the thickness of the heel portion of the mattress and a fifth actuator varies the thickness of the remainder of the foot portion of the mattress. The second actuator is
5 deactivated when it encounters a predetermined resistance. Preferably, this is during rotation down.

A control system includes an angle sensor and a length sensor connected to the foot section of the deck. Also, a foot prop sensor is connected to the foot section of the deck. As the length sensor senses the position of the end of the bed
10 or it's length, the appropriate inflation or deflation of the bladders is made to adjust the length of the foot portion of the mattress. The angle sensor cooperates with the foot prop sensor and the control system so that the foot section cannot pivot to an angle which will allow egress from the end of the bed without removal of the foot prop. This is preferably in the range of 65° to 90° from horizontal.

15 The foot prop has at least one foot support surface and means are provided for mounting the foot support surface to the foot section of the deck at different distances from the end of the foot section. The mounting means includes one or a pair of sockets spaced along the length of the foot section to receive the foot prop. The foot prop may include a rod received in the sockets. The rod may be
20 mounted asymmetrical with respect to a pair of opposed foot support surfaces. By rotating the foot prop 180°, the foot prop can be mounted in the same socket and achieve an adjustment. Alternatively, the rod may be symmetrically located and the distance adjusted by selecting one of a pair of sockets spaced along the length of the second foot section. The foot prop provides support from the horizontal to a chair
25 position up to an egress range of foot section angle.

Another method of shortening the length of the foot support surface beyond that which is produced by shortening the foot section of the deck is to not shorten nor thin the mattress foot portion when the foot section of the deck is shortened. The foot portion of the mattress can then be folded up the support surface
30 of the foot prop. This decreases the distance of the foot support surface by the thickness of the mattress foot section.

-4-

The structure which allows adjustability of the length of the foot section of the deck includes a first section connected to the remainder of the deck and a second section movable relative thereto. Telescopic guides connect the first and second sections and the actuator also connects the first and second sections.

5 Preferably, the actuator is between a pair of spaced telescopic guides connected to the first and second sections. Also, preferably, the telescopic guides includes three telescopic elements. The second foot section has a generally U-shaped cross section encompassing part of the top and lateral sides of the first section. The first section is a trapezoid having a large and small oppose surfaces and the large surface is the top of
10 the first foot section. The foot section of the deck has a width smaller than the width of the remainder of the deck and the foot prop is mounted to lateral extensions of the foot section. The width of the foot section with the lateral extensions is substantially equal to the width of the remainder of the deck. Bumpers are also mounted to the lateral extensions.

15 To size a support surface of the bed to an occupant and provide heel management, the bed may be used in the following method. The length of the foot section with a foot prop thereon is adjusted until the foot prop is immediately adjacent the foot of an occupant on the support surface. The thickness of a portion of the support surface of the mattress below the heel of the occupant is reduced. The length
20 of the foot section of the deck and the foot portion of the mattress are adjusted simultaneously. The foot section of the deck is adjusted using the first actuator, the foot portion of the mattress is adjusted using a second actuator and the thickness of one of the portions of the mattress foot portion is reduced using a third actuator.

A mattress includes a foot portion and a body portion within a ticking.
25 The foot portion is secured to the ticking as an adjustable length. The foot section may either be corrugated foam of adjustable length or a plurality of bladders which are inflatable and deflatable to adjust the length. The bladders need not be secured to the ticking. The ticking includes at least one slot and the foot section includes a flap secured thereto and extends into the slot to secure the foot section to the ticking. The
30 ticking includes an interior pocket and the slot is in the interior pocket. Magnets secured to the ticking for securing the mattress to the bed may also be provided in the pockets. A plate is also mounted to the foam displaced from the flat and straps are

-5-

secured to the plate and join the foot section to the foot portion of the mattress to the body portion of the mattress. A slip cover is provided encompassing the foot section to allow easy movement of the foot portion relative to the ticking.

Other objects, advantages and novel features of the present invention will become apparent from the following detailed description of the invention when considered in conjunction with the accompanying drawings.

Brief Description of the Drawings

Fig. 1 is a schematic view of a patient on a bed with the foot section/portion fully extended;

Fig. 2 is a schematic view of a patient on a bed with the foot section/portion adjusted and illustrating the heel management according to the principles of the present invention;

Fig. 3 is a bottom view of the foot section of a mattress according to the principles of the present invention;

Fig. 4 is a perspective top view of the foot section of the deck according to the present invention and connected to the remainder of the deck;

Fig. 5 is a bottom exploded view of a foot section of the deck of Fig. 4;

Fig. 6 is a bottom perspective view of 180° with respect to the respective view of Fig. 5 of one section of the deck of Fig. 5;

Fig. 7 is a top perspective view of the detail of the foot prop socket and safety switch according to the principles of the present invention;

Fig. 8 is a perspective view of the rotating mechanism according to the principles of the present invention;

Fig. 9 is an exploded perspective view of a mattress according to the principles of the present invention;

Fig. 10 is a perspective view of a foam foot portion of a mattress according to the principles of the present invention;

Fig. 11 is a bottom view of the foot portion of Fig. 10;

Fig. 12 is a side view of the foot portion of Fig. 10 with a cover according to the principles of the present invention;

Fig. 13 is a bottom view of the foot portion of Fig. 12;

-6-

Fig. 14 is a partial perspective view of the foot end of a ticking for a mattress according to the principles of the present invention;

Fig. 15 is a perspective view of the foot section of the deck and a foot prop;

5 Fig. 16 is a perspective view of a modified foot section of the deck with a pair of foot prop sockets;

Fig. 17 is a view of the foot section of the deck shortened and the mattress foot section folded; and

10 Fig. 18 is a schematic of the fluid controlled circuit for the foot angle actuator.

Detailed Description of the Preferred Embodiments

As illustrated in the Fig., the bed will be discussed with respect to a deck 10 and a mattress 20 thereon. As illustrated in Fig. 4, the deck 10 includes a seat
15 section 12, a thigh section 14 and a foot section 16 mounted to a frame 18. The deck would also include, but not shown, a head section also connected to the frame 18. Since the present invention is directed specifically to the foot section 16, the other portion will not be described in detail. The foot portion 16 may be used on any deck structure.

20 The retracting foot section of the present invention can be retracted while the bed is in its horizontal bed position. This permits the caregiver to adjust the overall length of the bed in either the bed position or the chair position. The overall bed length can be shortened by about 12-14 inches (30.5-35.5 cm) to facilitate transport of the bed. In other words, the retracting foot section reduces the bed length
25 so that the bed can fit into smaller elevators. The shorter bed also has a smaller turning radius. The foot section can also be moved to its retracted position to save space during storage of the bed.

The retracting foot section of the present invention also decreases patient migration since the foot prop location may be adjusted to the height of the
30 patient. Therefore, the bed size can be customized for the patient. The bed also includes a shearless pivot linkage disclosed in U.S. Patent No. 5,715,548 issued February 10, 1998, the specification of which is incorporated herein by reference. The

-7-

combination of the shearless pivot with the retracting foot section and foot prop reduces patient migration toward the foot end of the bed as the bed articulates.

The mattress 20 illustrated in Figs. 1 and 2 includes a body support portion 22 and a foot portion 24. The foot section 24 includes a calf portion 26 which is variable in length and thickness and a heel portion 28 which is variable in thickness. One preferred embodiment of the mattress foot portion 24 is illustrated in Figs. 1-3 as including a plurality of bladders. A plurality of variable thickness bladders 30 is separated by variable length bladders 32. The heel bladder 28 is separated from one of the variable thickness bladders 30 by a variable length bladder 32. The uniaxial variable bladders are produced by gussets in the bladders.

Referring to Fig. 3, a control line 34 is connected to the foot mattress portion 24 and by line 36 to the first variable thickness bladder 30. A line 38 at the other end of the first bladder 30 is connected to the second bladder 30. Line 40 at the opposite end of the second bladder 30 connects the second bladder 30 to the third bladder 30. A control line 42 is connected to line 44 of the foot portion 24 which is connected at its other end to the heel bladder 28. A control line 46 is connected to the first variable length bladder 32. All of the variable length bladders 32 are connected about the periphery of the foot portion 24. A cover 48 for the foot portion is held together by snaps 50. Preferably, the cover 48 is a slip or a shear promoting material, for example, 30 denier ripstop nylon which aids the movement of the foot section in the mattress ticking. This removes the shearing between the occupant and the ticking as the length of the mattress is changed. A strap 51 is secured to the cover 50 by the snaps which are rivets and ties the foot section to an adjacent section 22 of the mattress.

The control lines 34, 42, and 46 are connected to a control module which selectively inflates and deflates the bladders. An example of the control module is that in U.S. Patent No. 5,666,681 issued September 16, 1997, which is incorporated herein by reference. From the connection, all of the variable thickness bladders 30 are inflated and deflated simultaneously, all of the variable length bladders 32 are also inflated or deflated simultaneously. Alternatively, each of the variable length bladders may be individually controlled with additional control lines or other flow control mechanisms. All three types of bladders are independently controlled.

-8-

The foot section 16 of the deck includes a first section 52 connected to the frame 18 and the remainder of the deck and a second section 54 movable along the plane of the section 52. A foot prop 56 is mounted to the second foot section 54 and extends transverse to the plane of the foot sections 52 and 54.

5 To size the bed to the patient and provide heel management, an occupant is placed on the top surface of the mattress 20 as illustrated in Fig. 1 with the calf of the patient resting on the foot mattress portion 24. The foot deck section 54 is retracted onto the deck foot section 52 until the foot prop 56 is adjacent the foot of the occupant as illustrated in Fig. 2. Simultaneously, the length adjusting bladders 32 are
10 deflated so that the length of the portion 26 of the mattress is decreased, placing the heel of the patient above the heel bladder 28. The heel bladder 28 is then deflated, decreasing its thickness such that the interference pressure on the heel of the patient is reduced. By independently controlling the length of the foot section of the deck, the length of the foot portion of the mattress, and the thickness of the heel portion of the
15 mattress, appropriate adjustment of the length of the bed is possible as well as heel management.

 The foot section 16 of the deck may be pivotally connected to the frame so as to allow the foot section to drop and to be used in various styles of beds or chair beds. A separate and distinct actuator would be provided for the pivotal movement as
20 well as the articulation of the other deck sections. This allows adjustment of the foot section for the length of a patient and heel management independent of articulation of the deck and mattress as well as reducing the length and thickness of the foot portion of the mattress as the deck is converted to a chair.

 The foot section 16 of the deck will be explained with respect to
25 references 4-8. The first foot section 52 includes a top wall 58 and a pair of opposed lateral side walls 60. Mounted to the bottom surface of top wall 58 by welding for example, are a pair of guide tubes 62. An intermediate guide tube 64 is telescopically received with tube 62 and an end guide tube 66 is telescopically received in intermediate guide tube 64. As will be discussed below, the end guide tube 66 is
30 secured to the second foot section 54. The pairs of telescopic guide tubes 60, 64 and 66 guide the relative movement of foot section 54 with respect to foot section 52. Plates 68 are connected between the guide tubes 62 and the bottom surface of the top

-9-

plate 58. Thus, the foot section 52 has a trapezoidal shape. This trapezoidal shape with the larger of the two parallel surfaces being the top wall 58.

Also mounted to the under surface of the top wall 58 of the foot section is a hinge plate 70 which mates with a hinge plate 72 mounted to the deck frame 18.

- 5 This pivotally mounts the foot section 16 of the deck to the frame 18. Mounted between the guide tube 62 is a pair of spaced end walls 74 and 76.

- The second foot section 54 includes a top wall 78, a pair of side walls 80 extending therefrom, and a pair of bottom walls 82 extending from side walls 80. The top, side, and bottom walls are made from one continuous piece of material. The
- 10 second foot section 54 is generally U-shaped with bottom flanges 82 forming a C-channel with the side walls 80 and top walls 78. Thus, the top and side walls of the foot section 54 encompass or surrounds a portion of the top and side walls of the foot section 52. The foot section 54 includes an end wall 84 connected to the top wall 78, the side walls 80 and the bottom walls 82. Tube mounting assembly 86 mounts one
- 15 end of the guide tube 66 to the end wall 84 of the foot section 54.

- The end wall 76 of the foot section 52 includes openings 87 and 88, best seen in Figs. 4 and 6, between the guide tube 62. An actuator 89 shown in phantom in Fig. 5 is connected to end wall 74 and has an input connections. The actuator 89 is preferably an air cylinder, and mounting connection 90 on end wall 74 is
- 20 connected to a control line (not shown). The other end of actuator 89 is secured to wall 76 by bracket 92 in the opening 88. Arm 94 extending from actuator 89 is secured to wall 84 of the second foot section 54 by bracket 96. The actuator 89 is between the guide tubes 62, 64 and 66. The pair of guide tubes 62, 64, and 66 provides uniform distribution of forces. Also, the guide tubes support the weight of
- 25 the occupant's feet and minimizes friction between the walls of the foot section 52 and 54. This prevents binding and rubbing between the foot section 52 and 54.

- Plastic wipers 98 are also connected to the underside of top wall 78 of the foot portion 54 to protect the sliding joint between the foot sections 52 and 54 and also to prevent the sheet and mattress from intrusion into the joint and jamming the
- 30 foot section adjustment.

The foot section 54 includes lateral extensions 100. Bushing 102 mounts a bumper or roller 104 to the lateral extension 100. Socket 106 which receives

-10-

the foot prop 56 is also included in the lateral extension 100. Alternatively, a pair of sockets 106 and 107 may be provided on each extension 100 as shown in Fig. 16. A switch 108 is mounted to the socket 106 by fastener 110 as illustrated in Fig. 7.

- Switch 108 indicates the presence of the foot prop in the end of the bed and is part of the control system. Alternatively, the switch 108 may be designed to also sense the presence of pressure on the foot prop produced by the foot of the occupant of the bed engaging the foot prop of the occupant of the bed.

- Handles 128 are conveniently provided at the foot of the bed connected between the lateral extensions 100 and the foot section 54. A cover 150 is mounted to the end wall 84 of the foot section 54 as shown in Fig. 5. Slots 154 in the top of end wall 84 receives a stop 156 when the foot portion 24 of the mattress is made of foam as illustrated in Figs. 10-13.

- The width W1 of the foot sections 52 and 54 is substantially the width of the frame 18 and smaller than the width W2 of the frame 18 with its support surfaces. This accommodates side rails (not shown) mounted on the frame 18 in their lowered or tucked position as the foot section 16 pivots down. Width W3 of the foot section 16 with the lateral extensions 100 may be substantially equal to the width W2, since the extensions will pivot below the side rails.

- The length of the foot deck section 16 as well as the angle of the foot section 16 with respect to the frame 18 are determined by length sensor 114 and angle sensor 116 mounted to the first foot section 52 at tube 62 by bracket 112. A sensor crank 118 is mounted to the length sensor 114 at one end and its other end is mounted to sensor link 120. The sensor link 120 extends through the opening 87 in the wall 76 and is connected at its other end to a pivotal connection 122 to the end wall 84 of the foot section 54. The length sensor 114 may be for example, a potentiometer wherein the crank 118 and link 120 rotate the potentiometer with a change of the length of the foot section 54 with respect to foot section 52.

- A link 124 is connected to the angle sensor 116 at a first end by crank 123 and is pivotally connected at the second end to pivot leg 126 (shown in Fig. 6) mounted to hinge plate 72 (Fig. 4) which is connected to the deck frame 18. The angle sensor 116 may also be a potentiometer to determine the pivotal position of the foot section 16 with respect to the deck frame 18.

-11-

A pair of links 130 is pivotally mounted at one end to bracket 132 which is mounted to end wall 76 of the first foot section 52. The other end of links 130 are pivotally connected between brackets 134 and 136 mounted onto rod 138. The other end of brackets 136 is pivotally connected by brackets 140 to end wall 142 of the frame 18. Brackets 144 in the midsection of rod 138 connect rod 146 of actuator 148 to the rod 138. The other end of the actuator 148 is connected to the frame 18. A cover 150 has one end (not shown) connected to the frame 18 and its other end connected to brackets 152 which are mounted on end face 142 of the frame 18.

The actuator 148 determines the articulation or angular position of the foot section 16 of the deck. The actuator 148 illustrated in Fig. 18 includes rod 146 connected to piston 147. A pump 210 is connected to the opposite sides of piston 147 by raising valve 212 and lowering valve 214. Connected between the pump 210 and the valves 212 and 214 are filters 216, restriction 218, and check valves 220. Check valves 220 prevent the pressurized fluid in the actuator 148 from flowing back towards pump 210. The other side of piston 147 is connected to reservoir 222 by lowering return valve 224 and raising return valve 226. Filter 228 connects the reservoir 222 to the return valves 224 and 226 and a filter 230 connects reservoir 222 to the pump 210.

To extend the rod 146, electrical valves 212 and 226 are actuated to connect the respective sides to the pump 210 and reservoir 222. This raises the foot section 16. To lower the foot section 16, and retract the rod 146, electrical valves 214 and 224 are activated to respectively connect the opposite sides of the piston 147 to the pump 210 and reservoir 222. As a safety feature, relief valve 232 is connected between the output of pump 210 and the reservoir 222. Thus, if the pressure at the output of the pump builds up to an unsafe level, relief valve 232 provides a flow back to the reservoir 222.

As another safety feature, a relief valve 234 is connected between the output of valve 214 and the reservoir 222. Since valve 214 provides the output of the pump to the piston 147 to lower the foot section, if the pressure in the lowering should exceed the setting of relief valve 234, the excess pressure will be relieved back to reservoir 222. This is a safety feature in that if the foot section 16 engages an object in its lowering, the piston 147 and rod 146 will stop moving and pressure will build up on

-12-

that side of the piston. To prevent crushing of an object or a person or part of a person, relief valve 234 will operate. As an alternative to the relief valve 234, a pressure sensor may also be provided and the valve 214 may be closed or valve 226 opened. By way of example only and not by way of limitation, whereas the relief valve
5 232 for the pump may be set at 900 PSI (620.5 N/cm²), the relief valve 238 for the actuator 148 may be set at approximately 180 PSI (124.1 N/cm²).

The electronics portion 160 of the controller as illustrated in Fig. 4 is mounted to the frame 18 below the seat section 12 and the thigh section 14 of the deck. The controller 160 is connected to the length sensor 114 by wire 162, to angle
10 sensor 116 by wire 164 and to the prop sensor switch 108 by wire 166. The sensor crank 118 and sensor link 120 are hollow or U-channel and the wire 166 for the prop traverses the foot section 116 through the channel in the sensor crank 118 and sensor link 120. As the length sensor 114 sense the position of the end of the bed or it's length, the appropriate inflation or deflation of the bladders is made to adjust the
15 length of the foot portion of the mattress. The angle sensor 116 in combination with the foot prop sensor 108 does not allow the foot section to pivot to an angle, for example in the range of 65° to 90° degrees from the horizontal, which will allow egress from the end of the bed without removal of the foot prop. This prevents the occupant from standing on the foot prop. Any angle less than this range will provide foot
20 support in a chair position which is not selected for ease of egress.

Details of the mattress 20 is illustrated in Fig. 9. Ticking 170 receives the body portion 22 and a foot portion 24. Two examples of each portion are illustrated. The body portion 22 could include a foam seat portion 172 and a foam back portion 174. Alternatively, it may include a bladder seat section 176 and a
25 bladder back section 178. The foot section 24 could include a foam foot portion 180 or the bladder foot portion 28, 30 and 32 of Fig. 3. The control lines 34, 42, and 44 have a bend which corresponds to the juncture of the back and seat section of the mattress where a majority of the bending of the mattress occurs. Any combination of feet section may be used with any combination of seat and back section.

30 The body portion 22 and the foot portion 24 fit within the ticking 170. The ticking 170 is a stretchable, breathable thermal plastic which is impervious to bacteria. The seams of the outer ticking of the mattress are formed by continuous

-13-

ultrasonic welding. Therefore, the seams do not require any stitches which can permit fluid leakage. The ultrasonically welded seams are impermeable to fluids and bacteria so that the seams of the ticking prevent leakage into an interior region of the mattress.

Magnets 182 are provided at the foot end and the head end of the
5 ticking 170 in interior pockets 184 as illustrated in Fig. 14. These magnets secure the foot and head end of the bed to the frame or deck. If the frame is metal, no additional magnets are needed. If not, magnets are also provided on the supporting deck or frame.

The details of the foam foot portion 180 is illustrated in Figs. 10-13. A
10 foam core 186 is corrugated along its length or longitudinal axis. Preferably, the foam is low-ILD, visco elastic foam. Its ILD is in the range of 8-12 and is preferably 10. The length of the foam foot portion 186 may be, for example, 27 inches (68.58 cm) and is capable of being shortened to 13.5 inches (34.29 cm). This is an example of one foot portion. The corrugation allows the foot portion to diminish in length. Also, the
15 load-ILD allows the foot portion to compress upon the weight of the patient. This will help reduce the pressure on the heel. Also, by providing one of the valleys adjacent to the foot end of the foot portion 186, the heel may rest in the valley and therefore offer a valley or decreased area under the heel.

A portion of the foam 186 adjacent to the remainder of the deck is
20 tapered at 188. This mates with a tapering 173 of the foam seat portion 172. This is to accommodate articulation between the foot portion and the seat or thigh portion. The foot end of the foam 186 has tapered corners 190. This allows them to lay adjacent to the foot prop 56.

Bonded to the bottom of the core 186 adjacent to the deck end is a
25 torque plate 192, as illustrated in Fig. 11. Prior to bonding, half of a male/female snap rivets 194 are inserted through the torque plate 192. An attachment plate 196 is also bonded to the bottom of the core 186 adjacent to the foot end. Only the cross-half section is bonded and the ends are left free as flaps.

The core 186 is provided within a slip cover 198 which includes a
30 zipper 200 as illustrated in Figs. 12 and 13. The cover 198 preferably is a shear promoting material, for example, 30 denier ripstop nylon which aids the movement of the foam foot portion in the ticking 170. The flaps of attachment plate 196 extend

-14-

through slots 202 in the bottom of the slip cover 198. This secures the foot end of the core 186 to the slip cover 198. The other end of the core 186 is secured within the cover 198 by snap rivets 206 extending through straps 204 and to be received in the mating snap 194 of the torque plate 192. The straps 204 secure the foam of the foot portion 180 to the adjacent seat portion of the mattress within the ticking 170. The flap ends of the attachment plates 196 extending through the cover 198 are also received in slots 208 of pockets 184 as are the magnets 182 of Fig. 14.

As illustrated in Fig. 15, the foot prop 56 has opposed foot support surfaces 55 and 57. The general shape of the foot prop 56 is trapezoidal in cross-section. The distance D between the parallel surfaces 55 and 57 may be, for example, 2 ½ inches (6.35 cm). A pair of rods 59 extends from the bottom surface of the foot prop 56 and is received in sockets 106 in the second foot section 54. Although the foot section 16 is shortened or retracted when the deck rotates from its flat or planar position to the chair position, for very short occupants, the foot prop 56 would still not provide support for the feet of the short occupant. In such a case, the foot prop 56 can be rotated 180° with respect to that shown in Fig. 15 such that the planar surface 57 would be the foot support surface. It would be 2 inches (5.08 cm) closer to the patient than if surface 55 was the foot support surface.

As an alternative, a pair of sockets 106 and 107 spaced along the length of the foot section may be provided in each extension 100 as illustrated in Fig. 16. The distance E between the sockets 106 and 107 again, may be, for example, 2 ½ inches (6.35 cm). This will allow the foot prop 56 to be moved from sockets 106 to sockets 107 and thereby shortening the end by 2 ½ inches (6.35 cm). Rotating the foot prop 56 such that the surface 57 becomes a support surface, would shorten it an additional 2 inches (5.08 cm). Thus, an adjustment of 4 ½ inches (11.43 cm) can be obtained using the configuration of Fig. 16. Additional sockets may be provided to give additional adjustments.

It should also be noted that although the cross section of the foot prop 56 is shown as trapezoidal, any cross sectional configuration which provides a differential between the two opposed supporting foot surfaces may be used.

It is important that the foot prop 56 has the parallel surface 55 as a support surface when the deck is in its planar position and that it is in sockets 106. Otherwise,

-15-

it would overlap the mattress and prevent the end section from inflating to the appropriate height. Sensors and controls can be provided in the sockets 106 and 107 as well as some sensible indicia on 59 to indicate which socket it is in and which surface, 55 or 57 is adjacent the foot. Once this is sensed, the inflation of the foot section would be prevented until either the foot prop 56 has been removed or it is in socket 106 with surface 55 being the foot support surface. Also, as previously discussed, the control should not allow the foot section to rotate beyond, for example, 65° with respect to the horizontal if the foot prop is mounted in either of the sockets 106 or 107. This allows the foot prop to be available when the foot section is in a chair position while preventing it from being used when the foot section is lowered to permit egress.

Another method of changing the position of the foot support surface of the foot prop 56 greater than that achieved by the adjustment of the foot section 16 of the deck is illustrated in Fig. 17. While the foot section 16 is adjusted from its extended to its contracted shortened position, the mattress foot portion 24 is not shortened nor made thinner. The non-shortened portion of the foot portion 24 of the mattress then extends up one of the support surfaces of the foot prop 56 and forming a foot support surface. If the thickness of the foot portion 24 of the mattress 20 is, for example, five inches (12.7 cm), this will shorten the length of the foot section by five inches (12.7 cm). Also, if the reversible foot prop, as illustrated in Figs. 15 and 16 is used, this would add an additional 7 ½ to 9 ½ inches (19.05 to 24.13 cm) of adjustment.

Although Fig. 17 illustrates further decreasing the length of the deck in the planar or total horizontal position, the same adjustment can be made as the foot section of the deck and mattress are rotated down from the horizontal position towards the chair position. The controller would have to be modified so as to not simultaneously adjust the height or length of the foot section of the mattress 24 during the rotational and shortening of the foot section of the deck.

Although the present invention has been described and illustrated in detail, it is to be clearly understood that the same is by way of illustration and example only, and is not to be taken by way of limitation. The spirit and scope of the present invention are to be limited only by the terms of the appended claims.

CLAIMS:

1. A bed comprising:
a deck having a foot section of variable length along a plane of the foot
5 section;
a foot prop mounted to a first end of the foot section and extending
transverse to the plane of the foot section;
a mattress on the deck and having a foot portion of variable length
along a plane of the foot portion and variable thickness transverse to the plane of the
10 foot portion; and
a heel portion of the mattress foot portion adjacent the foot prop having
a thickness variable independent of the thickness of the remainder of the foot portion.
2. A bed according to claim 1, wherein the foot portion of the
mattress includes a plurality of variable length elements separated by a plurality of
15 variable thickness elements.
3. A bed according to claim 2, wherein the variable length
elements are interconnected to operate simultaneously and the variable thickness
elements are interconnected to operate simultaneously.
4. A bed according to claim 2, wherein the heel portion, the
20 variable length elements and the variable thickness elements each include one or more
bladders which are inflatable and deflatable.
5. A bed according to claim 1, wherein the heel portion and the
remainder of the mattress each include one or more bladders which are inflatable and
deflatable.
- 25 6. A bed according to claim 1, wherein the foot section is pivotally
mounted to the deck.
7. A bed according to claim 6, including a first actuator varying
the length of the foot section of the deck, a second actuator pivoting the foot section
of the deck and a third actuator varying the length of the foot portion of the mattress.
- 30 8. A bed according to claim 7, including a fourth actuator varying
the thickness of the heel portion of the mattress and a fifth actuator varying the
thickness of the remainder of the foot portion of the mattress.

-17-

9. A bed according to claim 6, including an angle sensor and a length sensor connected to the foot section of the deck.

10. A bed according to claim 1, including a foot prop sensor and a length sensor connected to the foot section of the deck.

5 11. A bed according to claim 1, wherein the foot section of the deck includes a first section connected to the remainder of the deck and a second section movable relative to the first section; telescopic guides connecting the first and second sections and an actuator connecting the first and second sections.

10 12. A bed according to claim 11, wherein the actuator is between a pair of spaced telescopic guides connecting the first and second sections.

13. A bed according to claim 11, wherein the telescopic guides includes three telescopic elements.

15 14. A bed according to claim 1, wherein the foot section of the deck includes a first section connected to the remainder of the deck and a second section movable relative to the first section; and the second section has a generally U-shaped cross-section encompassing part of a top and lateral sides of the first section.

15. A bed according to claim 14, wherein the first section is trapezoidal having a large and small opposed surfaces and the large surface is the top side of the first section.

20 16. A bed according to claim 1, wherein the foot section of the deck has a first width smaller than a second width of the remainder of the deck and the foot prop is mounted to lateral extension of the foot section.

17. A bed according to claim 16, wherein a third width of the foot section with the lateral extensions is substantially equal to the second width.

25 18. An bed having an adjustable length deck, the deck comprising:
a first section connected to the remainder of the deck;
a second section movable in a plane relative to the first section;
a pair of spaced telescopic guides connecting the first and second sections; and

30 a first actuator connecting the first and second sections.

19. A bed according to claim 18, wherein the telescopic guides includes three telescopic elements.

-18-

20. A bed according to claim 18, wherein the actuator is between the pair of spaced telescopic guides.

21. A bed according to claim 18, wherein the second section has a generally U-shaped cross-section encompassing part of a top and lateral sides of the first section.

22. A bed according to claim 21, wherein the first section is trapezoidal having a large and small opposed surfaces and the large surface is the top side of the first section.

23. A bed according to claim 18, wherein the first and second sections of the deck have a first width smaller than a second width of the remainder of the deck; the second section includes lateral extensions and prop is mounted to lateral extensions and extends transverse to the plane.

24. A bed according to claim 23, wherein a third width of the foot section with the lateral extensions is substantially equal to the second width.

25. A bed according to claim 18, wherein the first section is pivotally mounted to the remainder of the deck; and including a second actuator connected to and pivoting the first section and means for deactivating the second actuator when it encounters a predetermined resistance.

26. A bed according to claim 18, including a prop mounted to the second section of the deck; a prop sensor connected to the second section; and a length sensor connected to the first section.

27. A bed having an adjustable length deck, the deck comprising:
a first section connected to the remainder of the deck;
a second section movable in a plane relative to the first section and having a generally U-shaped cross-section encompassing part of a top and lateral sides of the first section; and

a first actuator connected to the second section to move the second section relative to the first section.

28. A bed according to claim 27, wherein the first section is trapezoidal having a large and small opposed surfaces and the large surface is the top side of the first section.

-19-

29. A bed according to claim 27, wherein the first and second sections of the deck have a first width smaller than a second width of the remainder of the deck; the second section includes lateral extensions and prop is mounted to lateral extensions and extends transverse to the plane.

5 30. A bed according to claim 29, wherein a third width of the foot section with the lateral extensions is substantially equal to the second width.

31. A bed according to claim 29, including a bumper mounted on each of the lateral extensions.

32. A bed according to claim 27, wherein the first section is
10 pivotally mounted to the remainder of the deck; and including a second actuator connected to and pivoting the first section and means for deactivating the second actuator when it encounters a predetermined resistance.

33. A bed according to claim 32, including an angle sensor and a length sensor connected to the first section of the deck.

15 34. A bed according to claim 27, including a prop mounted to and extending transverse to the second section of the deck; a prop sensor connected to the second section; and a length sensor connected to the first and second sections.

35. A method of fitting a support surface of a bed to an occupant, the bed including an adjustable foot section and a foot prop extending up from the foot
20 section, the method comprising:

adjusting the length of the foot section until the foot prop is immediately adjacent feet of an occupant on the support surface; and

reducing a thickness of a portion of the support surface below heels of the occupant.

25 36. A method according to claim 35, wherein the bed includes a deck with an adjustable length foot section and a mattress with a foot portion including a plurality of adjustable length and thickness portions; the length of the foot section of the deck and the foot portion of the mattress are adjusted; and the thickness of one of the portions of the mattress foot portion is reduced.

30 37. A method according to claim 36, wherein the the length of the foot section of the deck is adjusted using a first actuator; the foot portion of the

-20-

mattress is adjusted using a second actuator; and the thickness of the one of the portions of the mattress foot portion is reduced using a third actuator.

38. A bed having an adjustable length deck, the deck comprising:
a first section connected to the remainder of the deck;
5 a second section movable in a plane relative to the first section;
a first actuator connected to the second section to move the second section relative to the first section;
a prop mounted to and extending transverse to the second section of the deck;
10 a prop sensor connected to the second section; and
a controller connected to the first actuator and the prop sensor.

39. A bed according to claim 38, wherein the first section is pivotally mounted to the remainder of the deck; and including a second actuator connected to the first section and the remainder of the deck.

40. A bed according to claim 39, including an angle sensor and a length sensor connected to the first section of the deck.

41. A bed according to claim 38, including a length sensor connected to the first and second sections.

42. A mattress comprising:
20 a foot portion and a body portion within a ticking; and
the foot portion being secured to the ticking and adjustable in length.

43. A mattress according to claim 42, wherein the foot portion is corrugated foam adjustable in length.

44. A mattress according to claim 43, wherein the ticking includes
25 at least one slot and the foot portion includes at least one flap secured thereto and extending into the slot to secure the foot portion to the ticking.

45. A mattress according to claim 44, wherein the ticking includes an interior pocket and the slot is in the interior pocket.

46. A mattress according to claim 45, including a magnet in the
30 pocket for securing the mattress to a bed.

-21-

47. A mattress according to claim 43, including a plate mounted to the foam and displaced from the flap, and straps secured to the plate and joining the foot portion to the body portion.

48. A mattress according to claim 42, wherein the foot portion is encompassed by a slip cover.

49. A mattress according to claim 42, wherein the foot portion includes a plurality of bladders which are inflatable and deflatable for length adjustment.

50. A mattress according to claim 42, including at least one magnet secured to the ticking for securing the mattress to a bed.

51. A mattress comprising:
a foot and body portion within a ticking;
the foot section being adjustable in length; and
a slip cover encompassing the foot portion.

52. A mattress comprising:
a foot and body portion within a ticking; and
magnets secured to the ticking for securing the mattress to a bed.

53. A mattress according to claim 52, wherein the magnets are secured interior the mattress.

54. A mattress comprising:
a foot and body portion within a ticking; and
the ticking being a breathable, liquid impervious thermal plastic having welded seams.

55. A bed according to claim 1, wherein the foot prop includes a rod which is received in a socket of the foot section and the rod is asymmetrical with respect to two opposed foot support surfaces of the foot prop.

56. A bed according to claim 55, wherein the foot section includes a pair of sockets spaced along the length of the foot section.

57. A bed according to claim 1, wherein the foot section includes a pair of sockets spaced along the length of the foot section and the foot prop includes a rod which is received in a socket of the foot section.

-22-

58. A bed according to claim 18, including a foot prop having at least one foot support surface and means for mounting the foot support surface to the second section of the deck at different distances from an end of the second section.

59. A bed according to claim 27, including a foot prop having at least one foot support surface and means for mounting the foot support surface to the second section of the deck at different distances from an end of the second section.

60. A bed according to claim 38, wherein the foot prop has at least one foot support surface and including means for mounting the foot support surface to the second section of the deck at different distances from an end of the second section.

61. A bed according to claim 1, wherein the foot portion is corrugated foam adjustable in length.

62. A bed having an adjustable length deck, the deck comprising:
a first section connected to the remainder of the deck;
a second section movable in a plane relative to the first section;
a first actuator connected to the second section to move the second section relative to the first section;
a prop mounted to and extending transverse to the second section of the deck; and

the prop has two opposed foot support surfaces asymmetrical with respect to the mounting of the prop to the second section of the deck.

63. A bed according to claim 62, wherein the foot prop includes a rod which received in a socket of the foot section and the rod is asymmetrical with respect to the two opposed foot support surfaces of the foot prop.

64. A bed according to claim 63, wherein the foot section includes a pair of sockets spaced along the length of the foot section.

65. A bed according to claim 62, wherein the first section is pivotally mounted to the remainder of the deck.

66. A method of adjusting a foot support surface extending up from a foot end of an occupant support surface of an occupant support, the occupant support includes a) a deck having an adjustable foot section and a foot prop extending up from the foot section adjacent the foot end and b) padding on the deck, having a foot portion and having the occupant support surface, the method comprising:

-23-

adjusting the length of the foot section of the deck with the foot prop to its shortest length; and

providing the foot support surface displaced from the foot end by at least one of a) repositioning, with respect to the foot section of the deck, a surface of the foot prop which is transverse to the occupant support surface to become the foot support surface and b) positioning a part of the foot portion of the padding adjacent the transverse surface of the foot prop such that the occupant support surface of the part of the foot portion becomes the foot support surface.

67. A method according to claim 66, wherein the foot prop has two opposed transverse surfaces asymmetrical with respect to the mounting of the prop to the foot section of the deck; and the repositioning of the foot prop includes rotating the foot prop 180 degrees and remounting to the foot section of the deck.

68. A bed having an articulated deck, the deck comprising:
a first section pivotally connected to the remainder of the deck;
a first actuator connected to the first section to pivot the first section relative to the remainder of the deck; and
means for deactivating the first actuator when it encounters a predetermined resistance.

69. A bed according to claim 68, including a second section movable in a plane relative to the first section; and a second actuator connected to the second section to move the second section relative to the first section.

70. A bed according to claim 68, wherein the first actuator is a fluidly driven piston and the means is a relief valve connected to the piston.

71. A bed according to claim 70, wherein the relief valve is fluidically responsive to fluid pressure on the piston.

72. A bed according to claim 70, including a sensor to sense the pressure on the piston and wherein the relief valve is an electro-fluid valve responsive to fluid pressure on the piston sensed by the sensor.

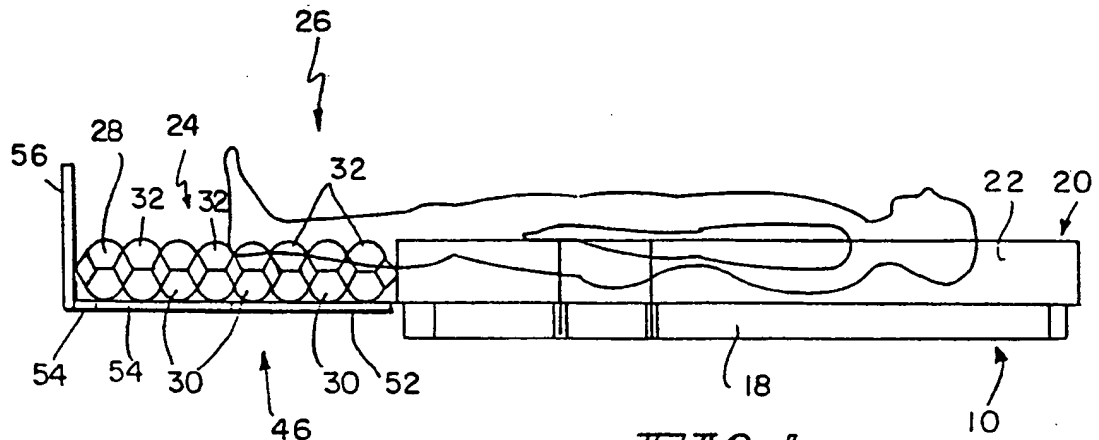


FIG. 1

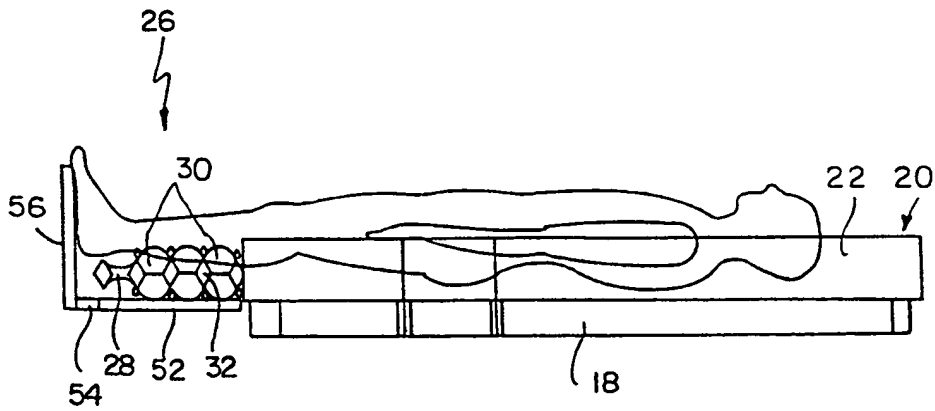


FIG. 2

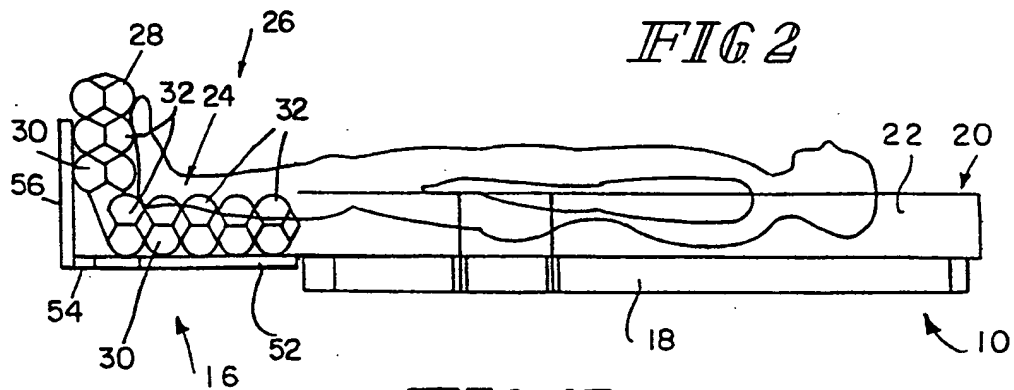
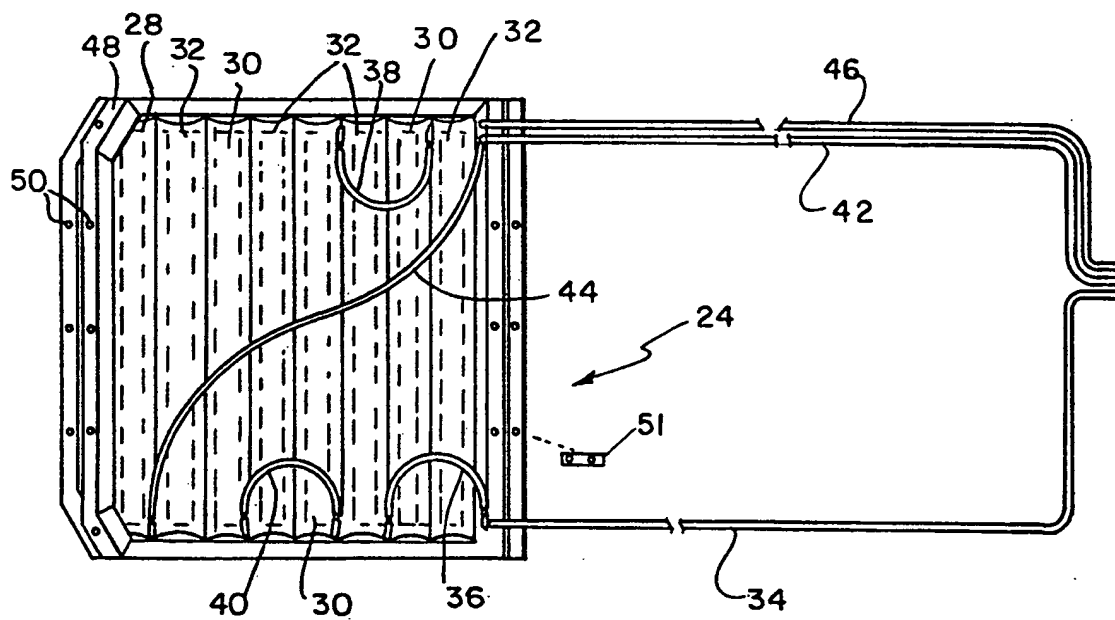
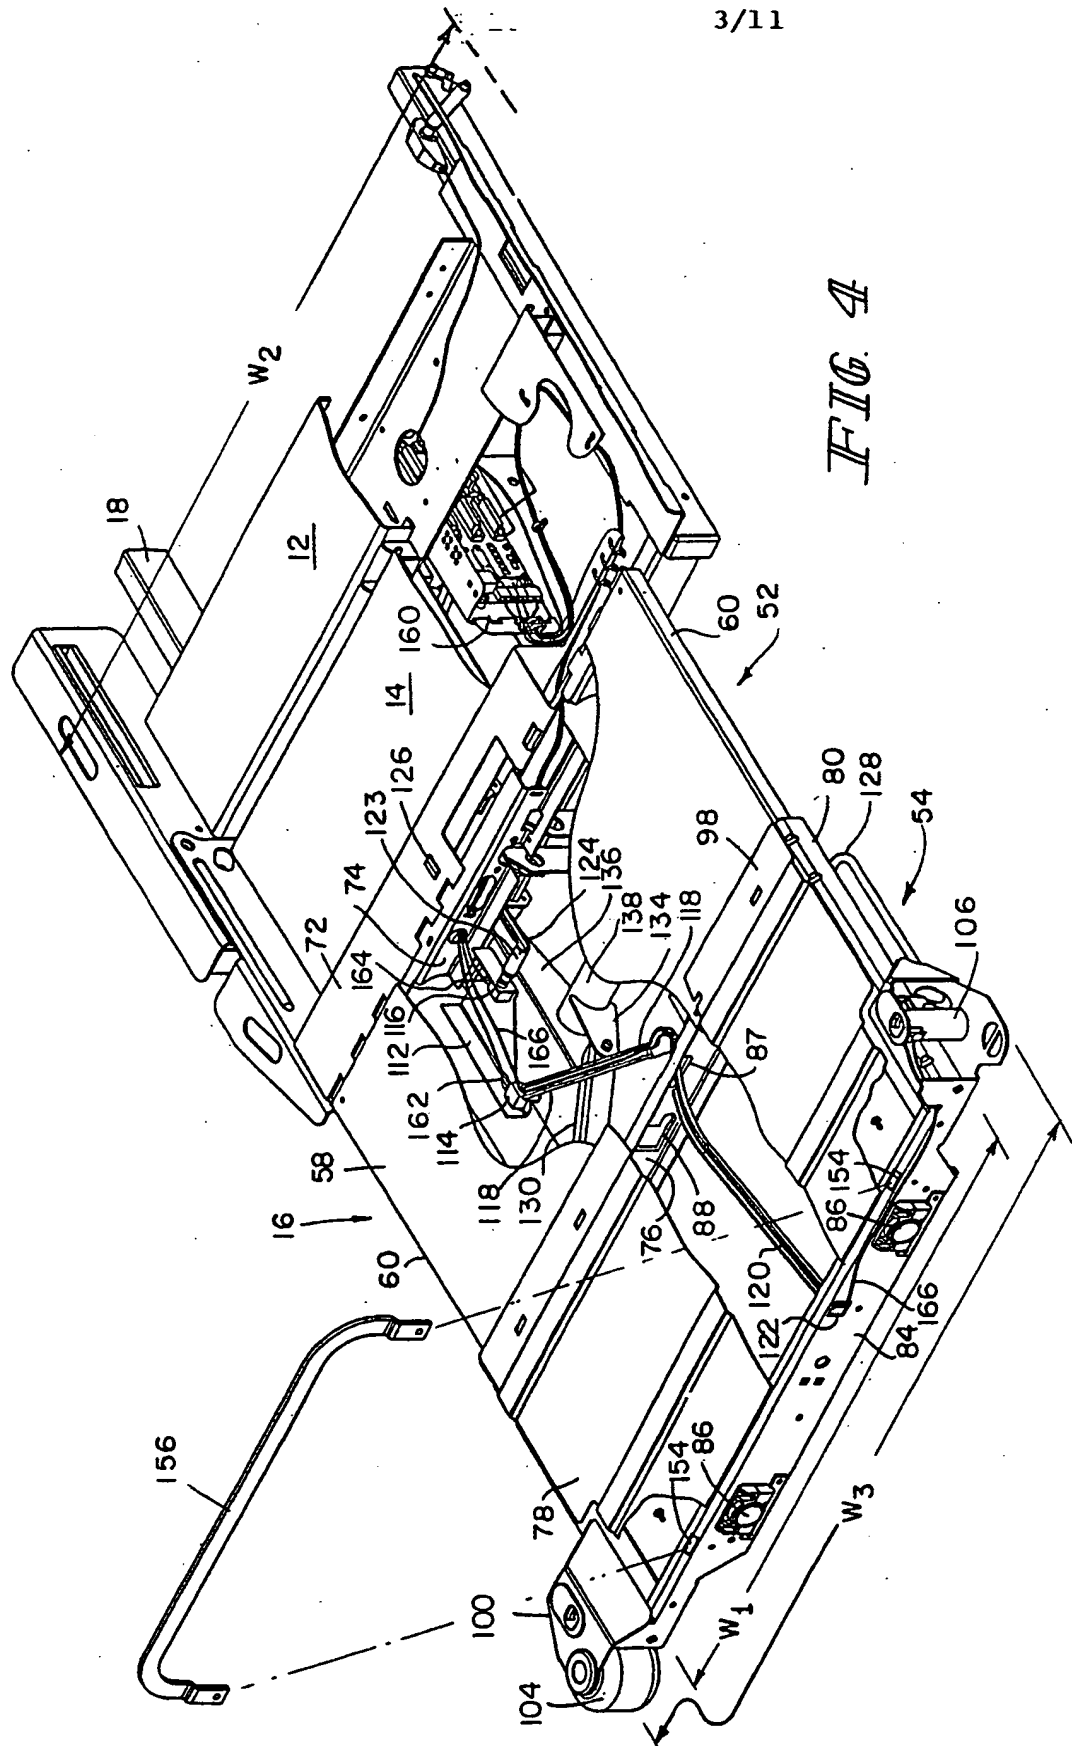


FIG. 17

2/11

*FIG 3*

3/11



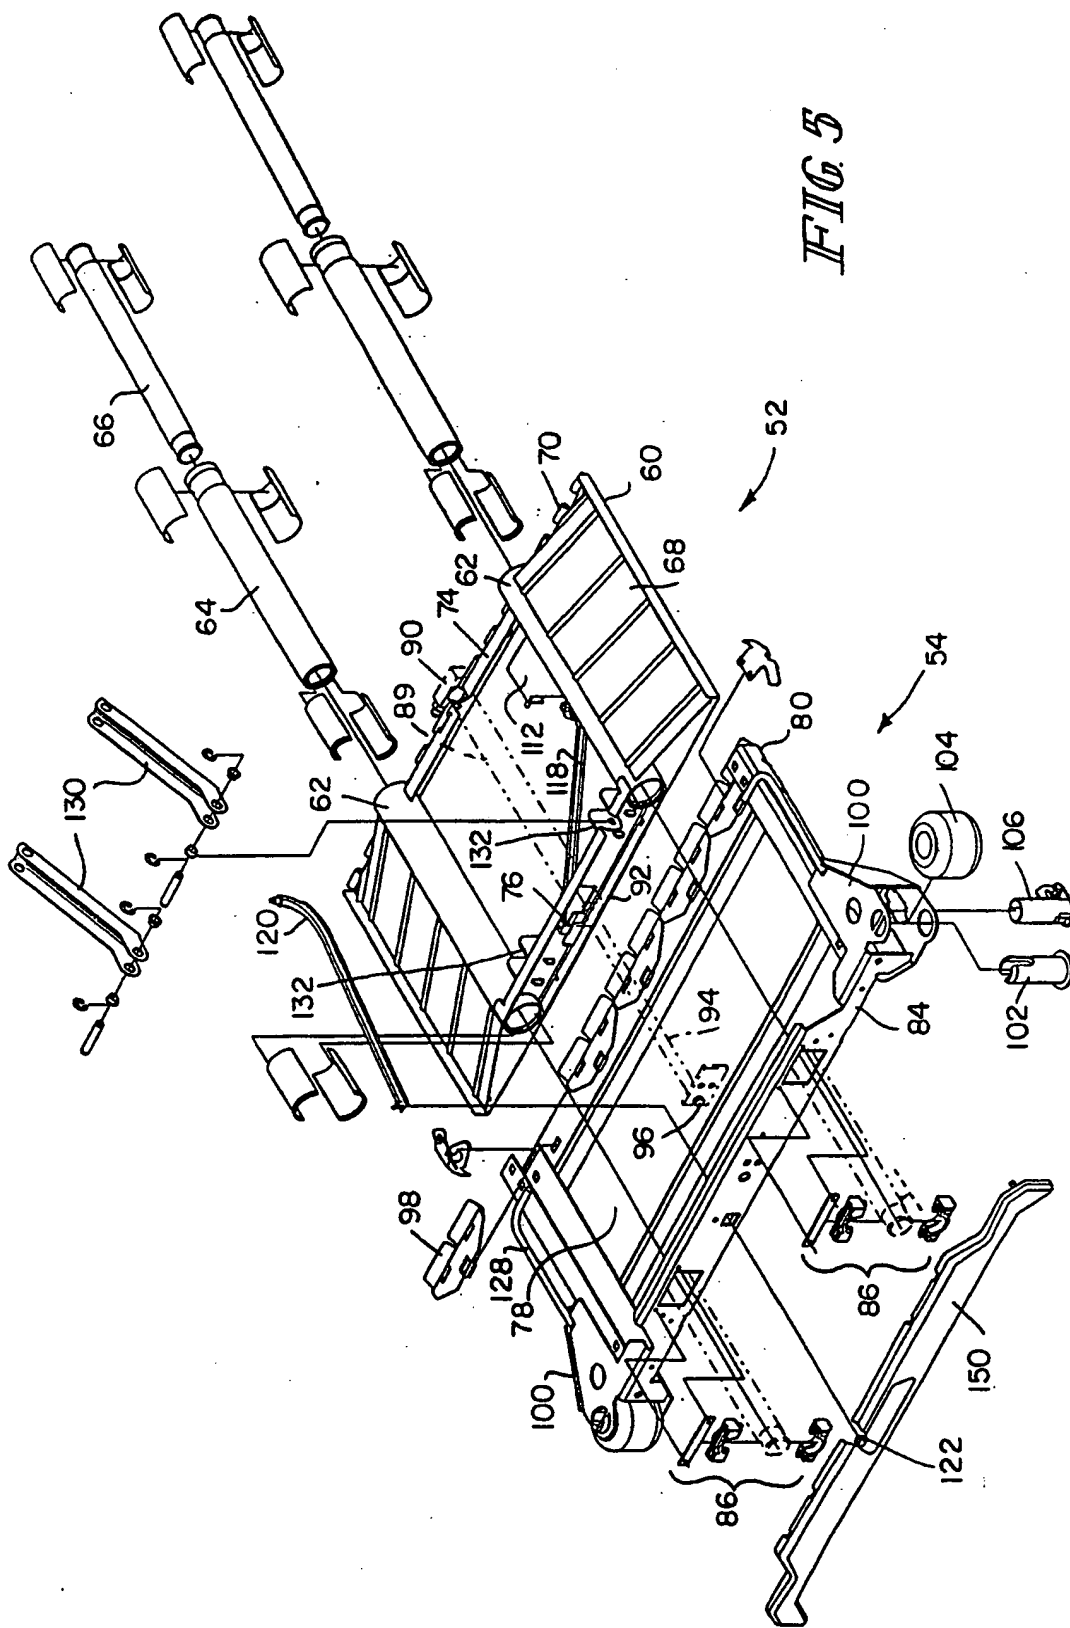


FIG 5

5/11

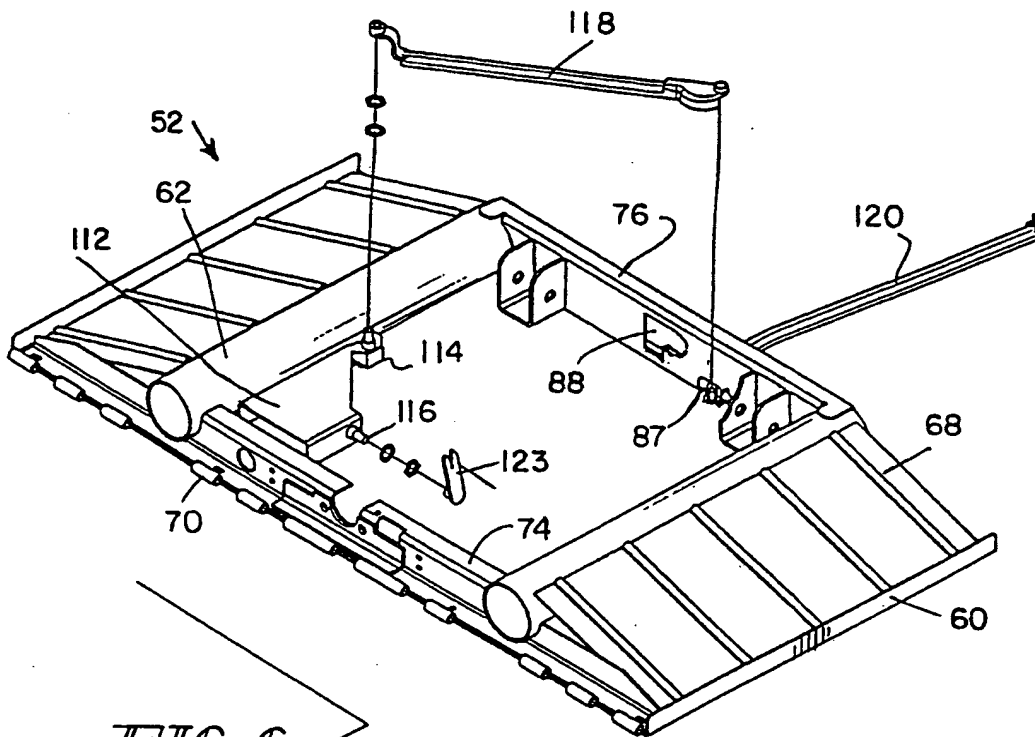


FIG. 6

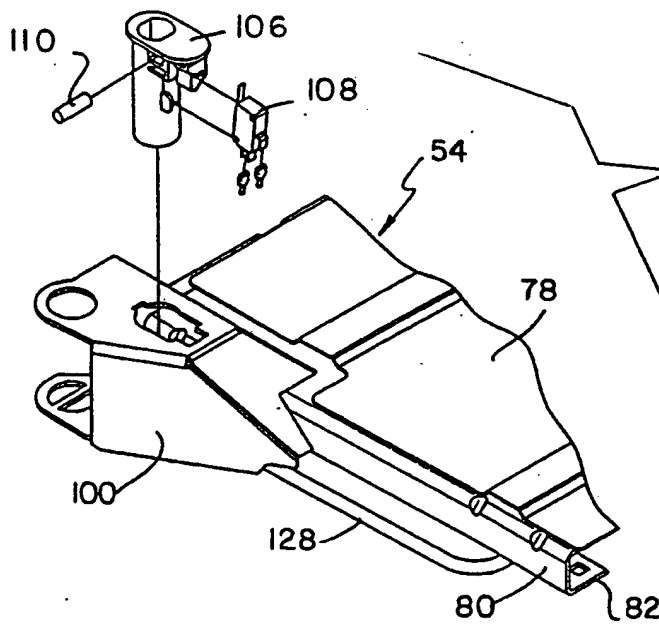



FIG. 7

6/11


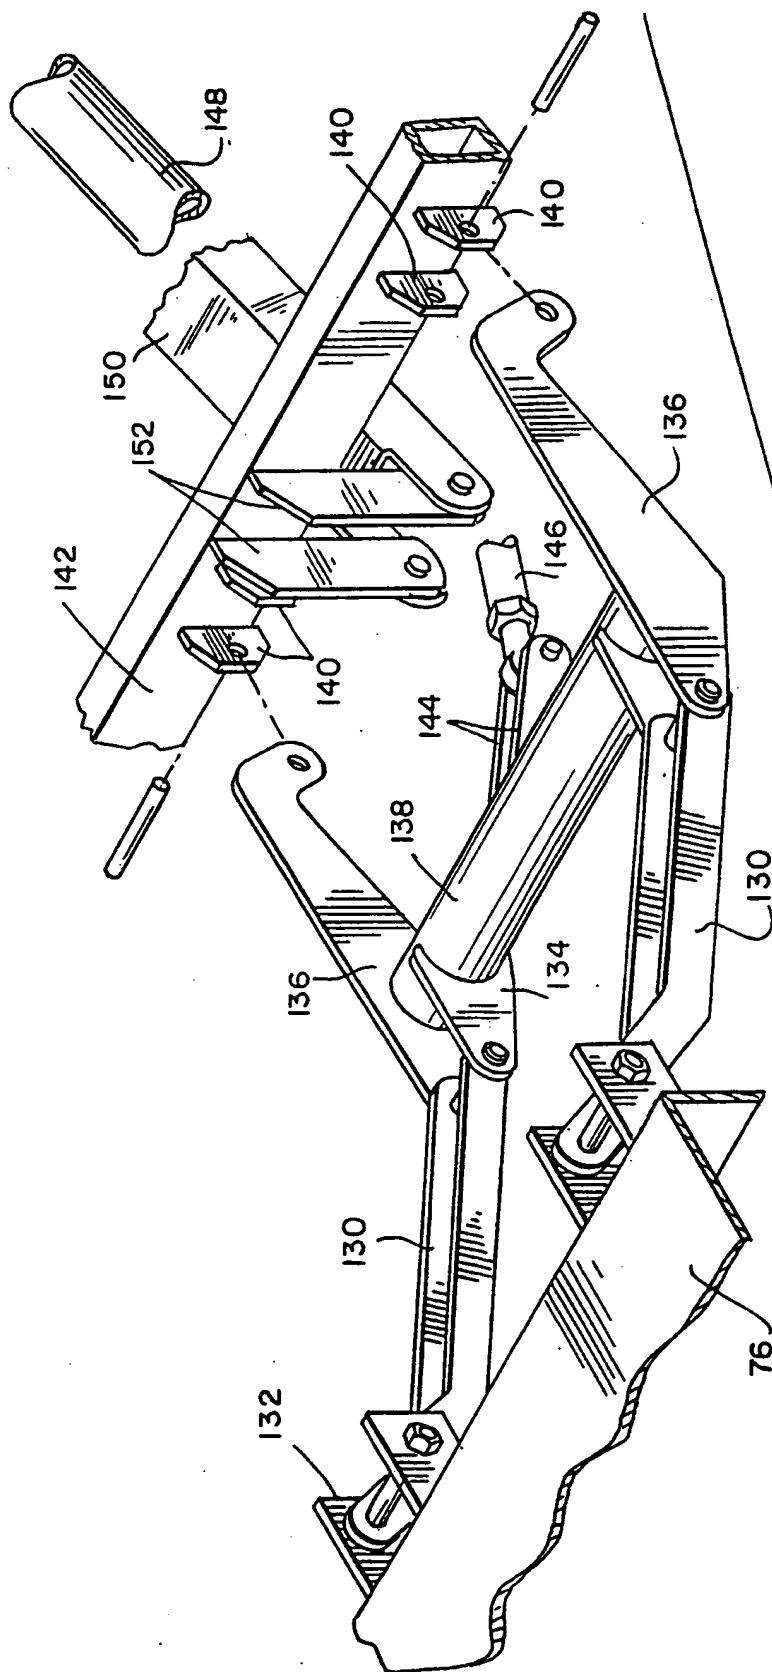


FIG 8

7/11

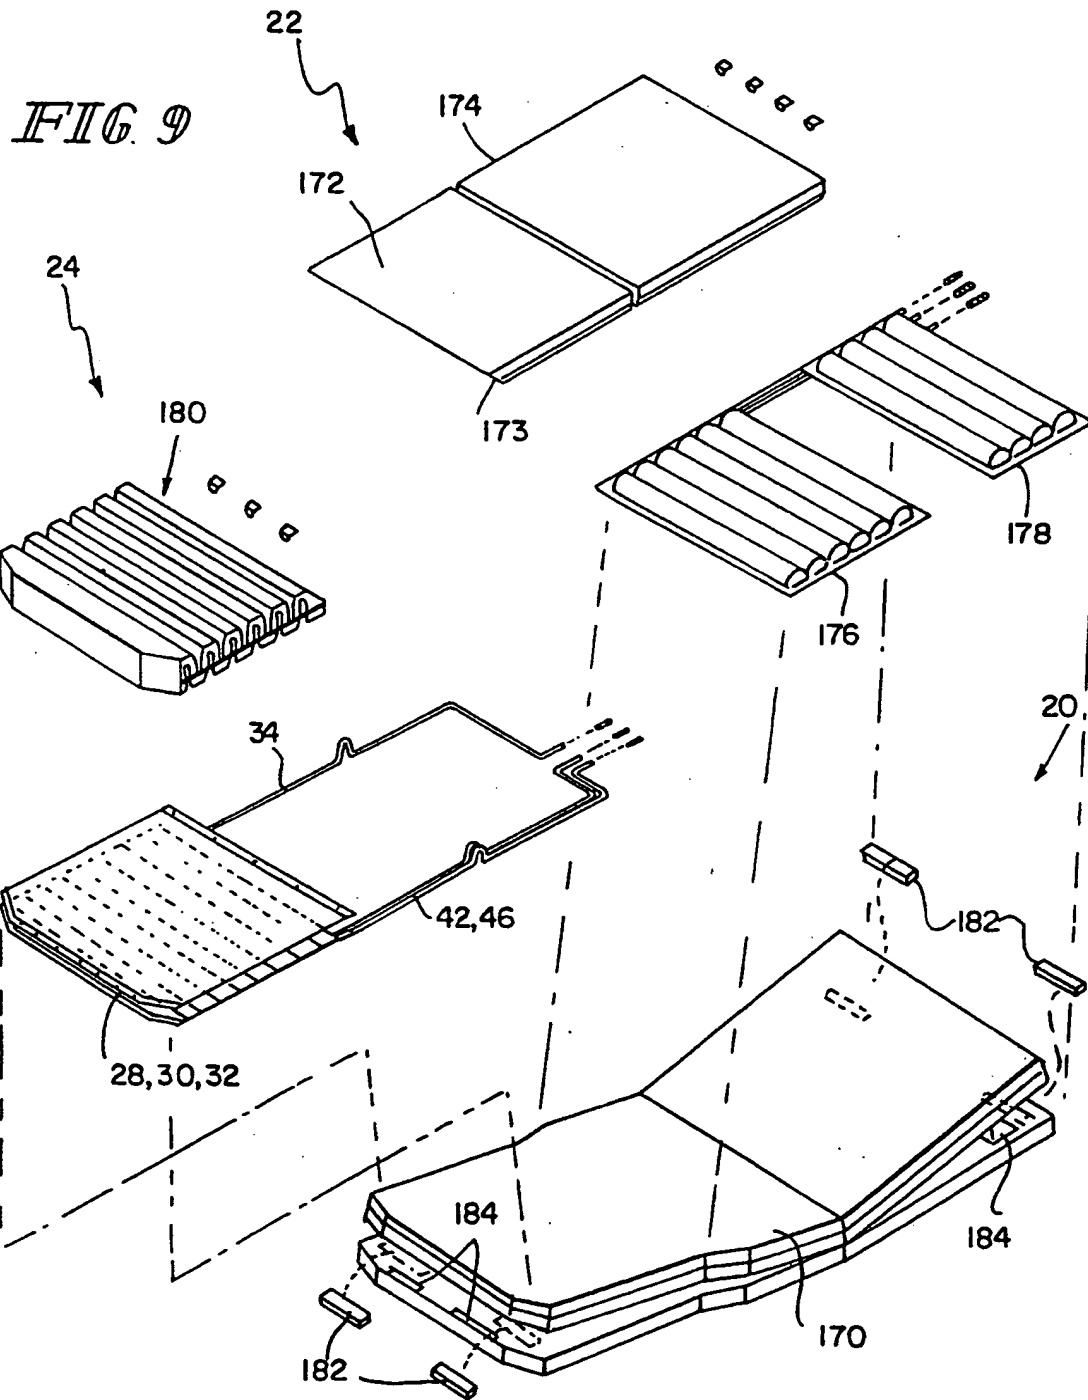

8/11

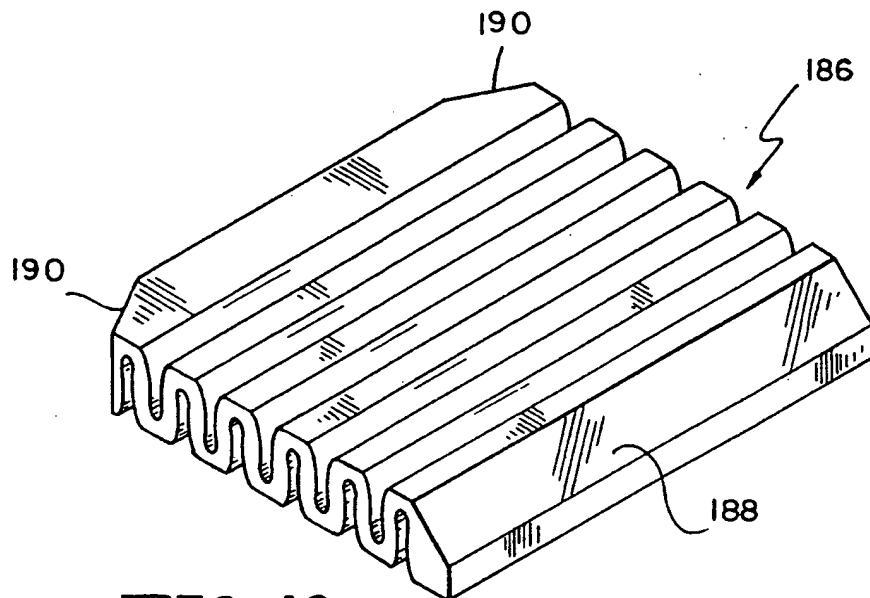


FIG. 10

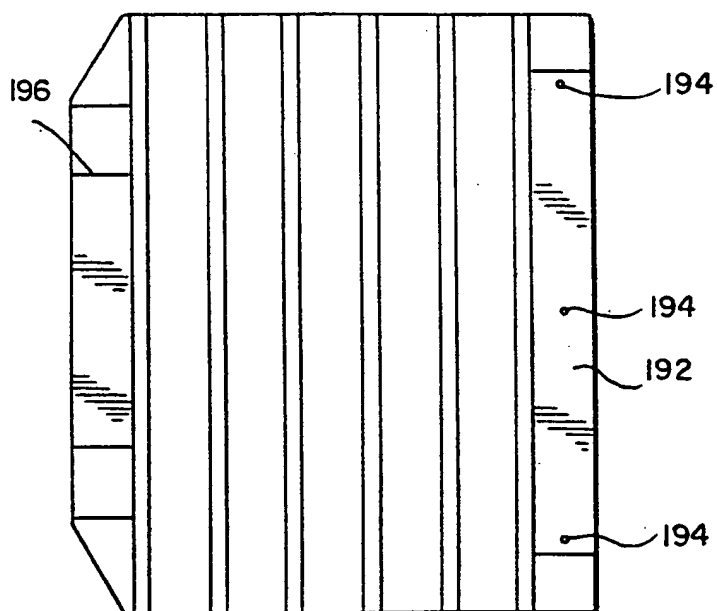


FIG. 11

9/11



FIG. 12

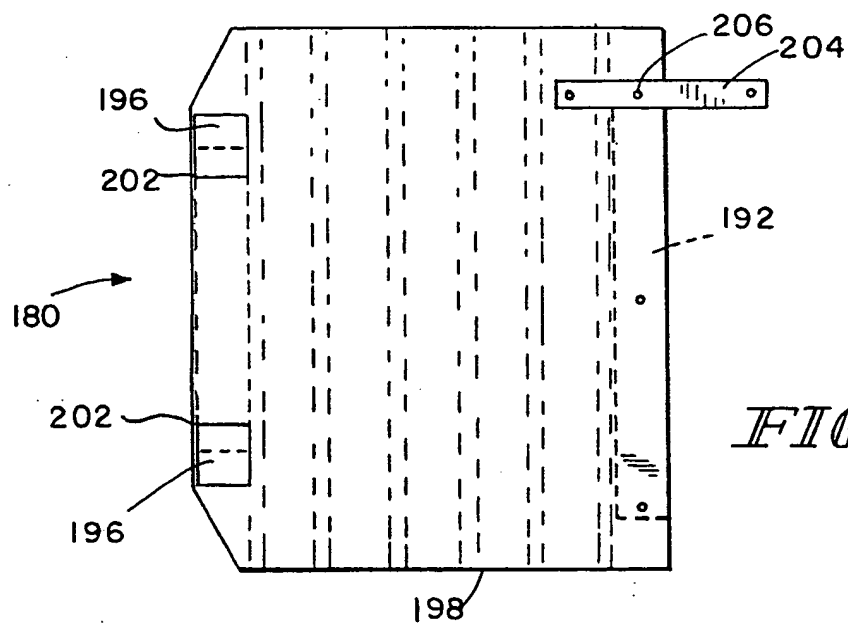


FIG. 13

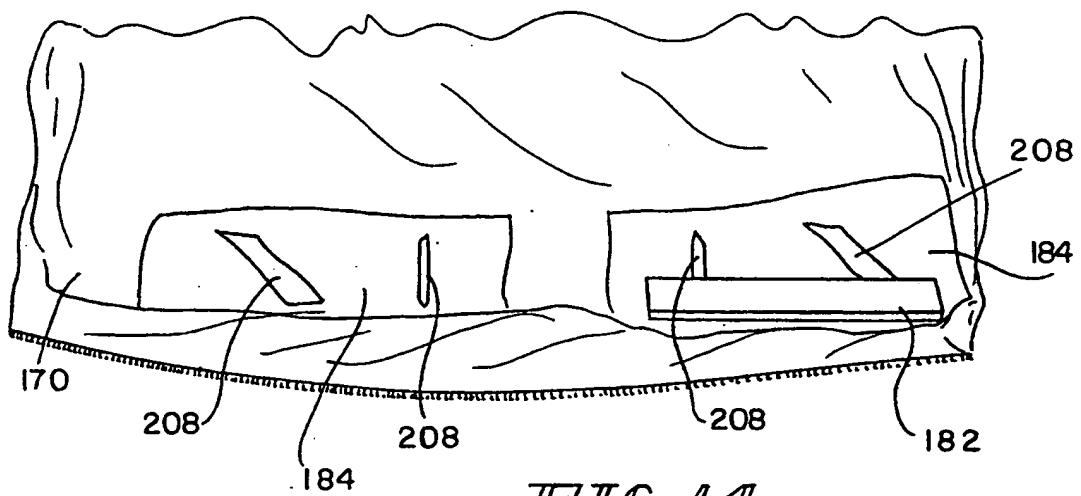
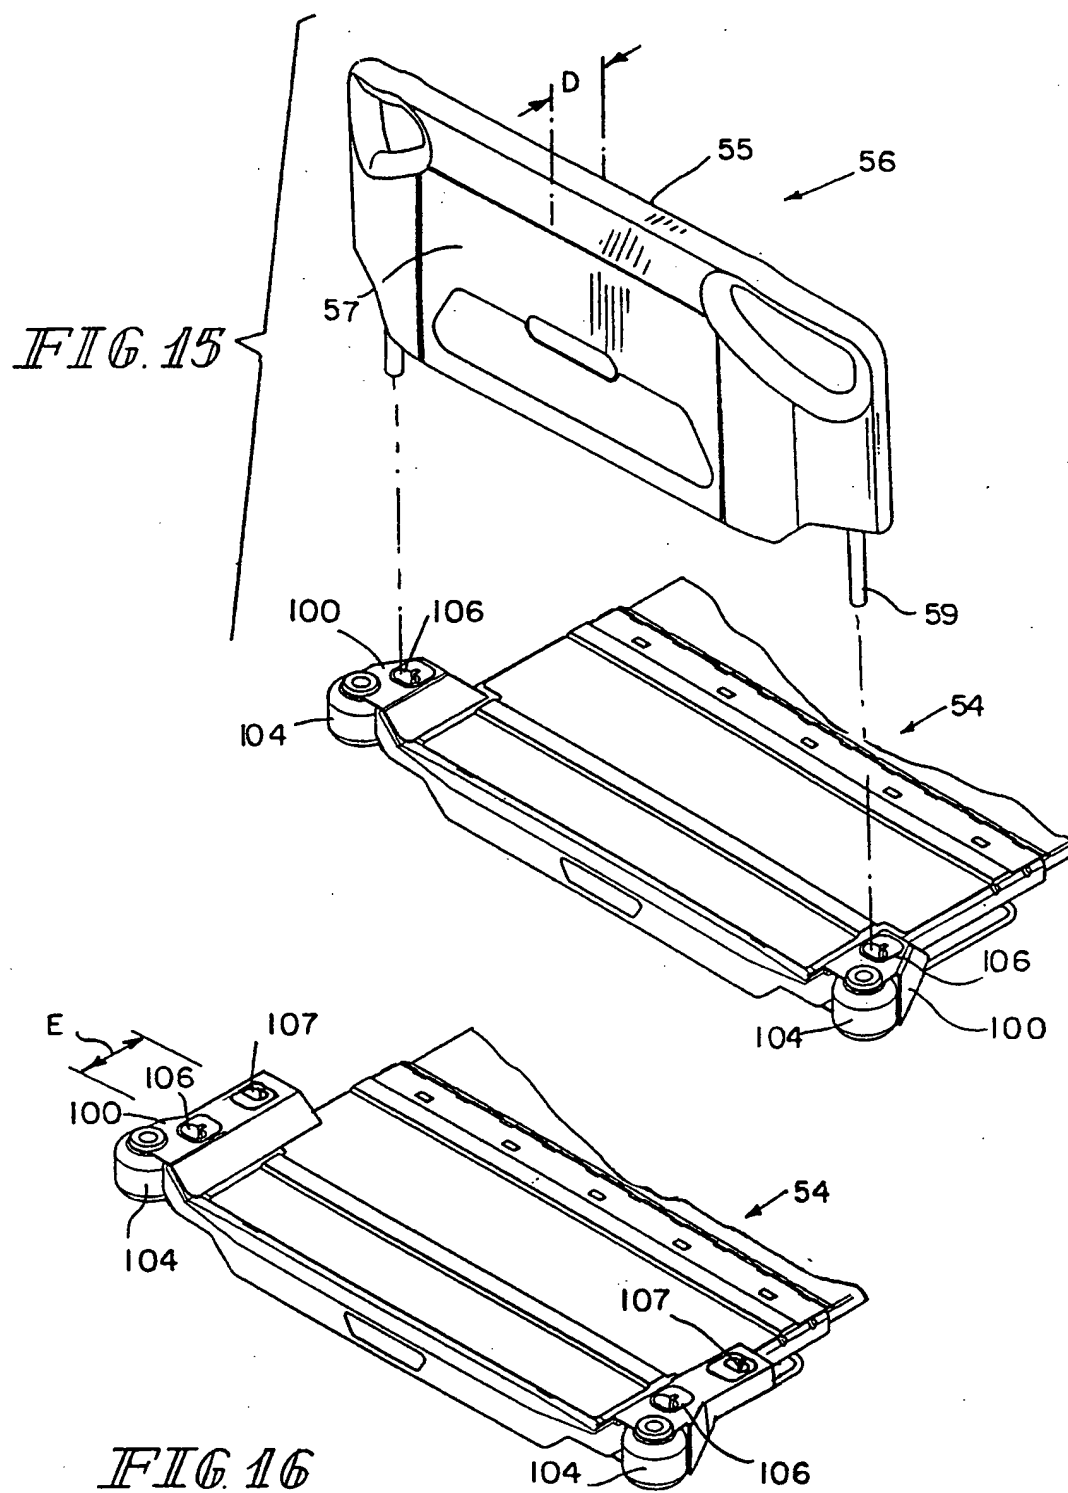


FIG. 14

10/11



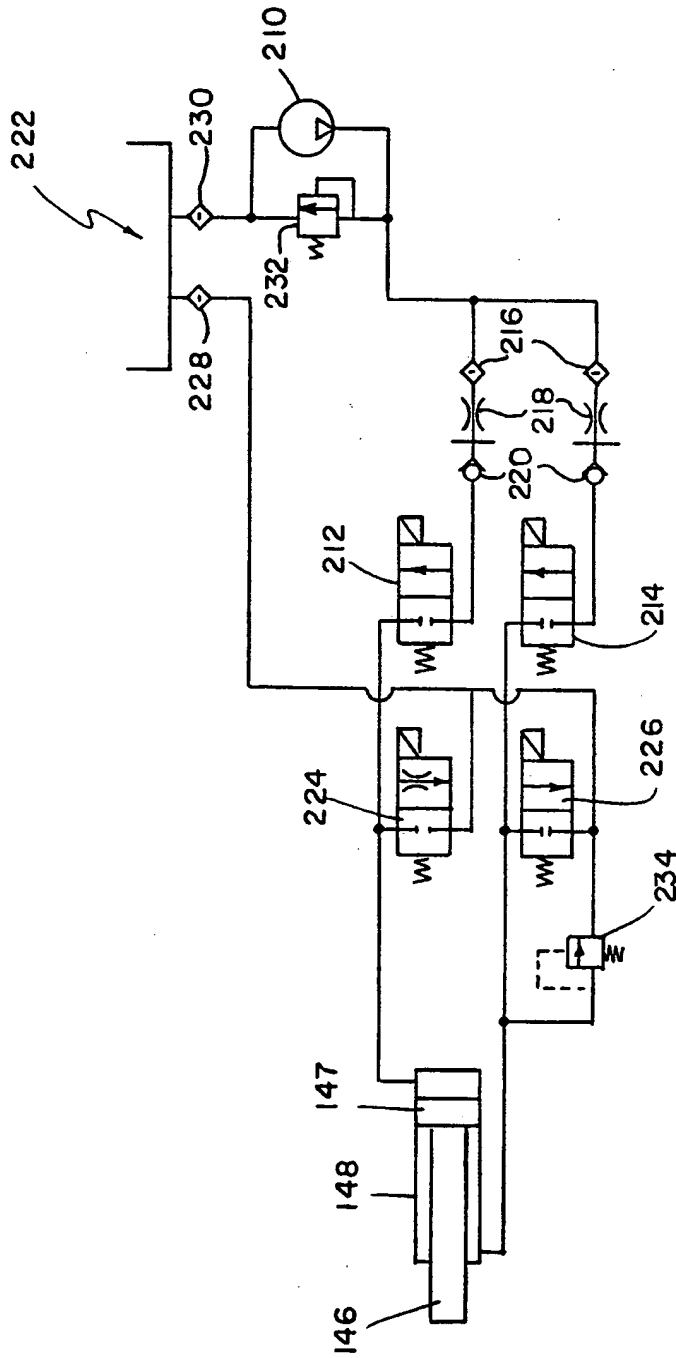



FIG. 18



INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification ⁶ : A61G 7/00, 7/057	A3	(11) International Publication Number: WO 99/15126 (43) International Publication Date: 1 April 1999 (01.04.99)
(21) International Application Number: PCT/US98/20002 (22) International Filing Date: 23 September 1998 (23.09.98) (30) Priority Data: 60/059,772 23 September 1997 (23.09.97) US 09/120,125 22 July 1998 (22.07.98) US (71) Applicant: HILL-ROM, INC. [US/US]; 1096 State Route 46 East, Batesville, IN 47006-9167 (US). (72) Inventors: ALLEN, E., David; 7513 South Dwyer, Okdana, OH 45053 (US). KRAMER, Kenneth, L.; 6769 West Bloomington Street, St. Paul, IN 47272 (US). WUKU-SICK, Peter, M.; 20157 Five Point Road, Batesville, IN 47006 (US). MEYER, Eric, R.; 4185 County Line Road, Greensburg, IN 47240 (US). BRANSON, Gregory, W.; 323 Woodfield Drive, Batesville, IN 47006 (US). ULRICH, David, J.; 22186 Ester Ridge Road, Sunman, IN 47041 (US). THOMAS, James, M., C.; 1486 Greenshade Way, Mt. Pleasant, SC 29464 (US). DANIEL, Paul, M., III; 2425 Venetian Way, Burlington, KY 41005 (US). ZWINK, Dennis, R.; 27105 Enochsburg Road, Batesville, IN 47006 (US).	(74) Agent: NIEDNAGEL, Timothy, E.; Barnes & Thornburg, 11, South Meridian Street, Indianapolis, IN 46204 (US). (81) Designated States: AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CU, CZ, DE, DK, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, UA, UG, UZ, VN, YU, ZW, ARIPO patent (GH, GM, KE, LS, MW, SD, SZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG). Published <i>With international search report.</i> (88) Date of publication of the international search report: 8 July 1999 (08.07.99)	

(54) Title: HOSPITAL BED HAVING A RETRACTING FOOT SECTION

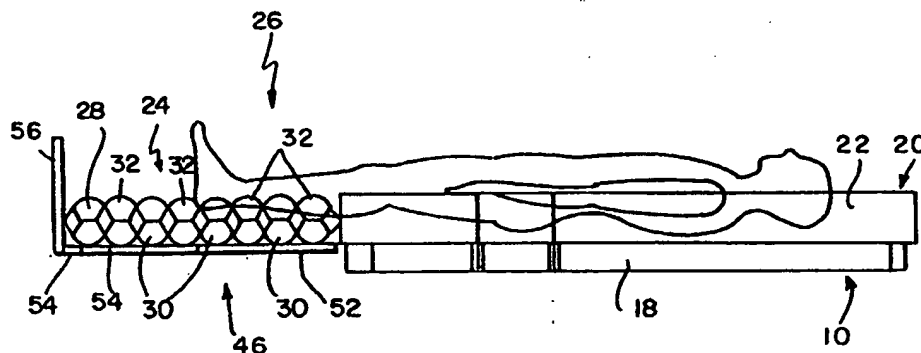

(57) Abstract

A bed having a foot prop (56) on an adjustable length deck foot section (52) and a mattress (20) with a length and thickness adjustable foot section (16) and a thickness adjustable heel section. The adjustability of the deck (10) and the mattress (20) allows sizing of the bed to the occupant as well as heel management. The foot prop (56) is also adjustable.

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece	ML	Mali	TR	Turkey
BG	Bulgaria	HU	Hungary	MN	Mongolia	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MR	Mauritania	UA	Ukraine
BR	Brazil	IL	Israel	MW	Malawi	UG	Uganda
BY	Belarus	IS	Iceland	MX	Mexico	US	United States of America
CA	Canada	IT	Italy	NE	Niger	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NL	Netherlands	VN	Viet Nam
CG	Congo	KE	Kenya	NO	Norway	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NZ	New Zealand	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	PL	Poland		
CM	Cameroon	KR	Republic of Korea	PT	Portugal		
CN	China	KZ	Kazakhstan	RO	Romania		
CU	Cuba	LC	Saint Lucia	RU	Russian Federation		
CZ	Czech Republic	LI	Liechtenstein	SD	Sudan		
DE	Germany	LK	Sri Lanka	SE	Sweden		
DK	Denmark	LR	Liberia	SG	Singapore		
EE	Estonia						

INTERNATIONAL SEARCH REPORT

International Application No

PCT/US 98/20002

A. CLASSIFICATION OF SUBJECT MATTER

IPC 6 A61G7/00 A61G7/057

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 6 A61G A47C F15B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	DE 23 10 603 A (BREMSHEY AG) 19 September 1974 see claim 1; figures ---	1, 18, 27, 35, 38, 62, 66
A	US 5 666 681 A (MEYER ERIC R ET AL) 16 September 1997 cited in the application see column 2, line 12 - line 14 see column 4, line 18 - line 44; figure 1 --- -/--	1, 18, 27, 35, 38, 42, 51, 62, 66



Further documents are listed in the continuation of box C.



Patent family members are listed in annex.

* Special categories of cited documents :

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier document but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

"&" document member of the same patent family

Date of the actual completion of the international search

14 April 1999

Date of mailing of the international search report

27. 04. 1999

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,
Fax: (+31-70) 340-3016

Authorized officer

GODOT, T

INTERNATIONAL SEARCH REPORT

Inter. Appl. Application No

PCT/US 98/20002

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT		
Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
P,A	US 5 715 548 A (ALBERSMEYER DAVID A ET AL) 10 February 1998 cited in the application	1,35,38, 42,51, 62,66
X	see column 52, line 50 - column 55, line 10; figures 24-25A	18,20, 21,27
Y	see figures 63-68	25,32, 68,69
X	US 2 605 151 A (SHAMPAINE) 29 July 1952 see column 4, line 21 - line 29; figures	18
A	US 3 845 947 A (LEE N) 5 November 1974 see abstract; figures	1,18,27, 35,38, 62,66
P,A	GB 2 313 303 A (EGERTON HOSPITAL EQUIP) 26 November 1997 see abstract; figures	1,18,27, 35,38, 62,66
Y	US 4 769 584 A (IRIGOYEN MARIO J ET AL) 6 September 1988 see abstract; figure 1	25,32, 68,69
X	US 5 235 258 A (SCHUERCH F WILLY) 10 August 1993	68
Y	see column 5, line 28 - line 36; figures 1,4	70-72
P,Y	US 5 701 618 A (BRUGGER KLAUS) 30 December 1997 see abstract; figure 1	70-72
A	EP 0 349 067 A (APPLIED POWER INC) 3 January 1990 see column 3, line 35 - line 41; figure 2	68,70-72
A	US 3 099 440 A (BURZLAFF) 30 July 1963 see column 3, line 19 - line 40; figures	68,70-72

INTERNATIONAL SEARCH REPORT

Int. l. application No.
PCT/US 98/20002

Box I Observations where certain claims were found unsearchable (Continuation of item 1 of first sheet)

This International Search Report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☐ Claims Nos.:
because they relate to subject matter not required to be searched by this Authority, namely:

2. ☐ Claims Nos.:
because they relate to parts of the International Application that do not comply with the prescribed requirements to such an extent that no meaningful International Search can be carried out, specifically:

3. ☐ Claims Nos.:
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box II Observations where unity of invention is lacking (Continuation of item 2 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

see additional sheet

1. ☐ As all required additional search fees were timely paid by the applicant, this International Search Report covers all searchable claims.

2. ☐ As all searchable claims could be searched without effort justifying an additional fee, this Authority did not invite payment of any additional fee.

3. ☒ As only some of the required additional search fees were timely paid by the applicant, this International Search Report covers only those claims for which fees were paid, specifically claims Nos.:

1-51,55-72

4. ☐ No required additional search fees were timely paid by the applicant. Consequently, this International Search Report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

Remark on Protest

- ☐ The additional search fees were accompanied by the applicant's protest.
- ☒ No protest accompanied the payment of additional search fees.

INTERNATIONAL SEARCH REPORT

International Application No. PCT/US 98/20002

FURTHER INFORMATION CONTINUED FROM PCT/ISA/ 210

This International Searching Authority found multiple (groups of) inventions in this international application, as follows:

1. Claims: 1-51,55-67

Bed with a deck having a foot section of variable length

2. Claims: 52,53

Mattress with magnets for securing to a bed

3. Claim : 54

Mattress with a breathable, liquid impervious ticking

4. Claims: 68-72

Bed having an articulated deck with means for deactivating the actuator

INTERNATIONAL SEARCH REPORT

Information on patent family members

Inter. Appl. No.

PCT/US 98/20002

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
DE 2310603 A	19-09-1974	AT 344314 B AT 164174 A CH 576769 A NL 7402795 A,B	10-07-1978 15-11-1977 30-06-1976 04-09-1974
US 5666681 A	16-09-1997	CA 2166442 A EP 0722683 A	04-07-1996 24-07-1996
US 5715548 A	10-02-1998	US 5479666 A AU 1909095 A CA 2182019 A EP 0744934 A JP 9508041 T WO 9519755 A US 5454126 A US 5577279 A US 5680661 A US 5708997 A	02-01-1996 08-08-1995 27-07-1995 04-12-1996 19-08-1997 27-07-1995 03-10-1995 26-11-1996 28-10-1997 20-01-1998
US 2605151 A	29-07-1952	NONE	
US 3845947 A	05-11-1974	GB 1436548 A AU 473084 B AU 5668873 A BE 800060 A CA 1000775 A CH 558174 A DE 2327028 A FR 2187281 A JP 49056490 A NL 7307644 A SE 390483 B ZA 7303511 A	19-05-1976 10-06-1976 12-12-1974 17-09-1973 30-11-1976 31-01-1975 20-12-1973 18-01-1974 31-05-1974 11-12-1973 27-12-1976 24-04-1974
GB 2313303 A	26-11-1997	NONE	
US 4769584 A	06-09-1988	NONE	
US 5235258 A	10-08-1993	NONE	
US 5701618 A	30-12-1997	DE 9317308 U AT 160500 T DE 59404682 D WO 9513043 A EP 0727977 A JP 2714720 B JP 8510678 T	16-03-1995 15-12-1997 08-01-1998 18-05-1995 28-08-1996 16-02-1998 12-11-1996
EP 0349067 A	03-01-1990	NL 8801644 A CA 1308626 A DK 322989 A FI 893123 A,B, JP 2052651 A US 4959957 A	16-01-1990 13-10-1992 29-12-1989 29-12-1989 22-02-1990 02-10-1990
US 3099440 A	30-07-1963	NONE	